


DEPENDENT ON THE PATIENT'S CLINICAL CASE<sup>1</sup>



LOW TO MEDIUM RISK

MEDIUM TO HIGH RISK

HIGH TO VERY HIGH RISK

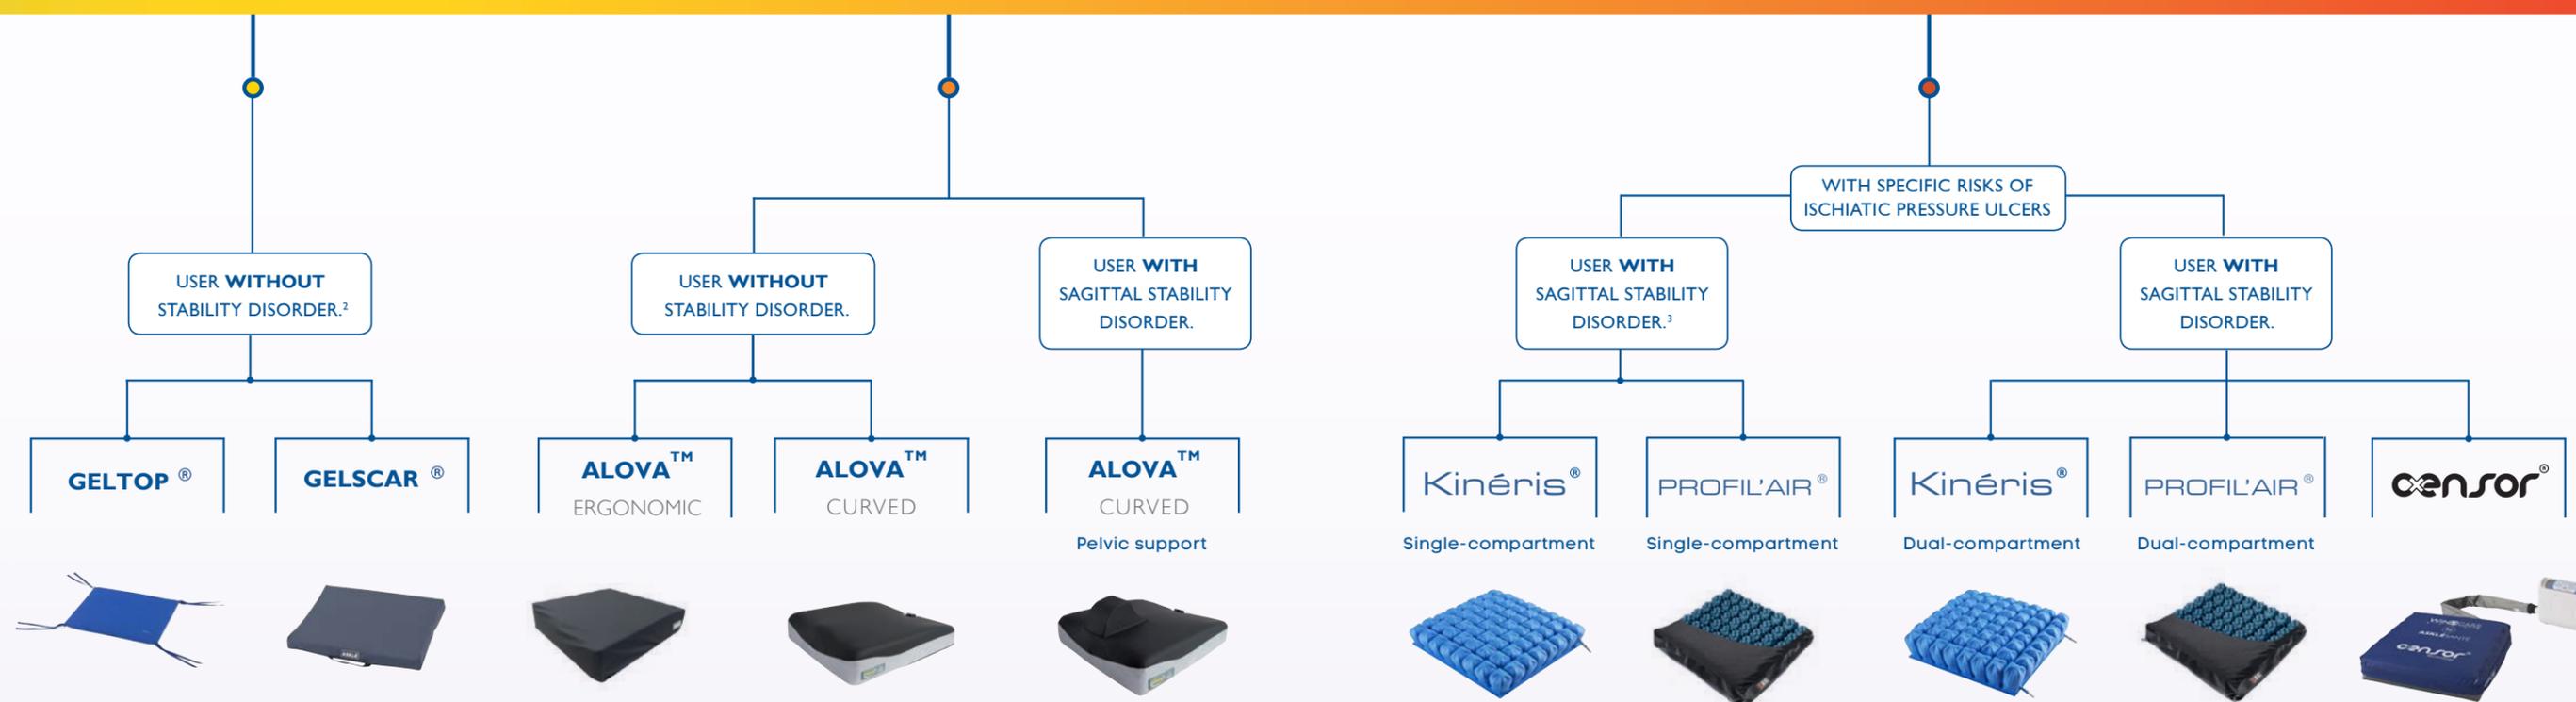

1 : Treatment aid on medical advice.

2 : Exclusion criteria for the "low to medium risk" category:

- History of ischial or sacro-coccygeal pressure ulcers
- Paralysis of the trunk and/or lower limbs
- Disorders of tenderness of the lower limbs
- Spasticity
- Support asymmetry (frontal or sagittal)
- Vascular amputee

3 : The prescriber must ensure that patients or their caregivers are able to adjust the support. The patient must be consulted by the prescriber in the following month.

These products are regulated Class 1 medical devices that bear the CE marking under this regulation. Carefully read the product instructions before use.

FP000098/01.2018

RISK ASSESSMENT ACCORDING TO CLINICAL OPINION AND VALIDATED SCALES

RISK	LOW TO AVERAGE	AVERAGE TO HIGH	AVERAGE TO HIGH
BRADEN SCALE	Score from 17 to 13	Score from 12 to 8	Score < 8
WATERLOW SCALE	Score from 10 to 15	Score from 15 to 19	Score from 20 and up
NORTON SCALE	Score from 14 to 12	Score from 11 to 9	Score from 8 to 5

Photos not contractually binding



WINNCARE Group : Aské Santé site - 200 rue Charles Tellier - Actiparc de Grézan - 30034 Nîmes Cedex 1 France  
Ph : +33 (0)4 66 02 15 15 - Fax : +33 (0)4 66 02 15 00 - Email : contact.aske@winnicare.fr - www.winnicare.fr

In the interest of constantly improving its products, the WINNCARE Group reserves the rights to modify the technical specifications of any product without prior notice.  
Class I medical device in accordance with European Directive 93/42/EEC

